

フタル酸エステルの分析

Analysis of Phthalates

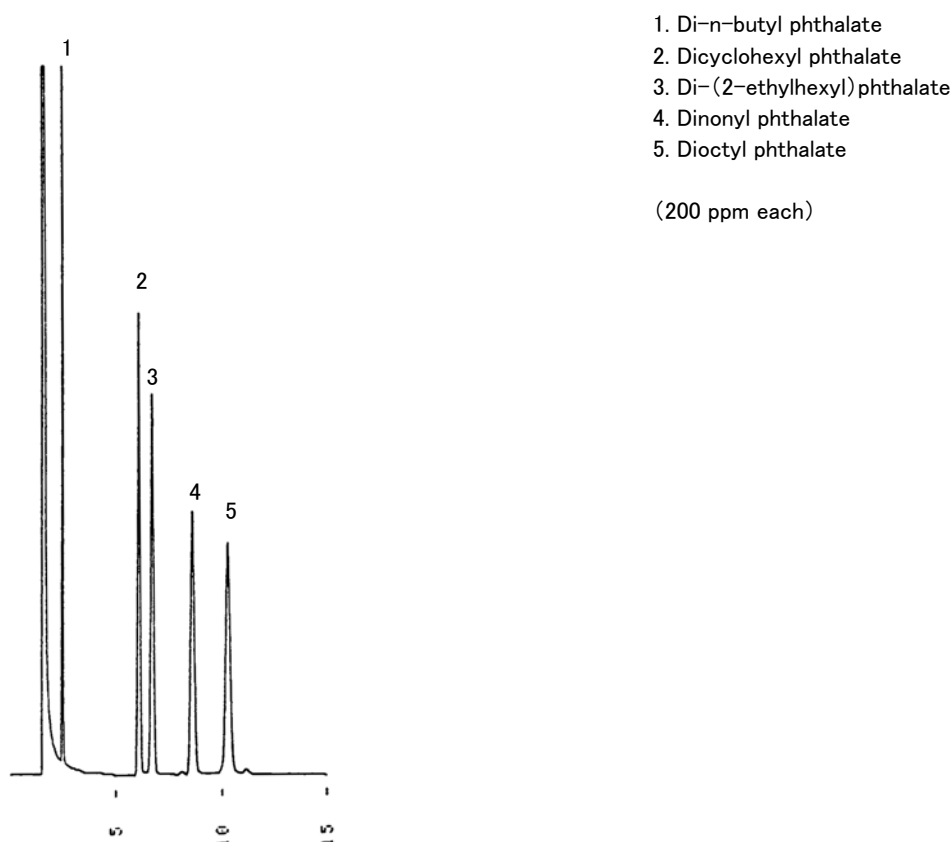


Fig. Chromatogram of Phthalates.

【Analytical conditions】

Column:	G-column G-100 40 m L. × 1.2 mm I.D. 0.5 μ m film thickness
Flow rate:	He 28 mL/min
C.Temperature:	240°C
Detection:	FID
Injection volume:	1 μ L
System:	-