

水中の低級アルコールの分析

Analysis of Lower alcohols in water

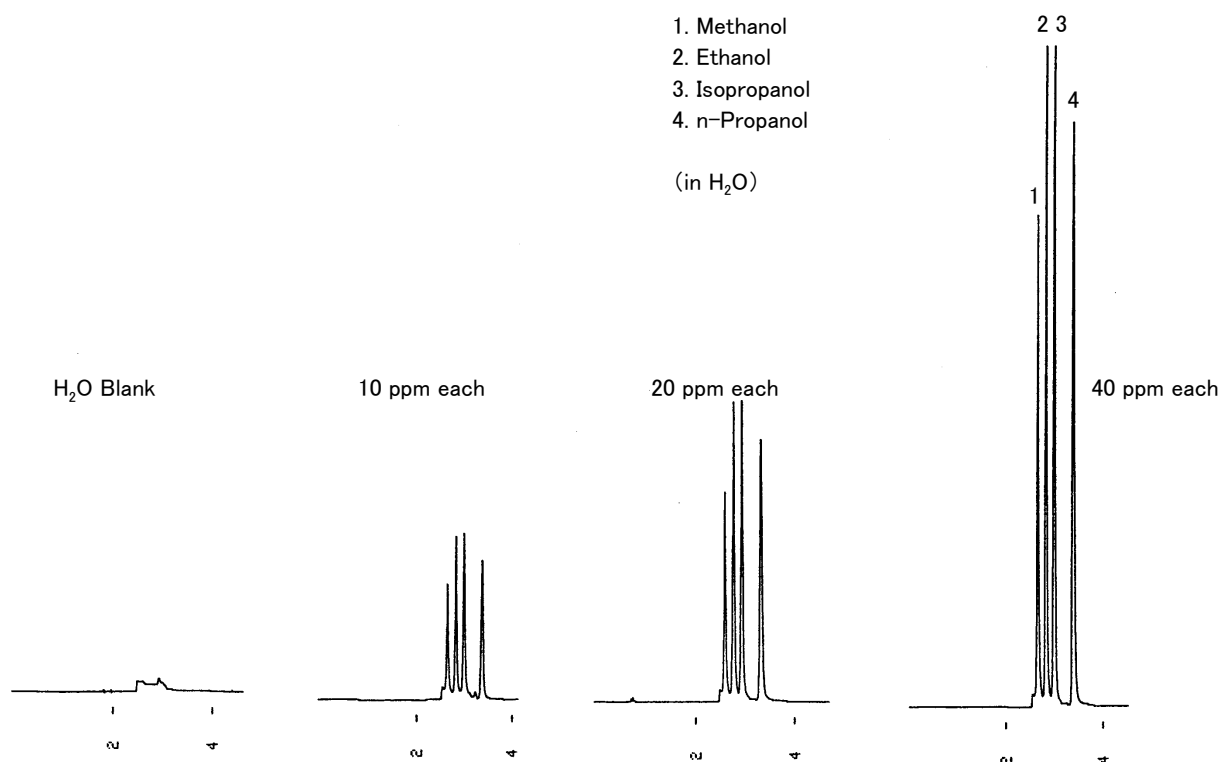


Fig. Chromatogram of lower alcohols in water.

【Analytical conditions】

Column: **G-column G-205** 40 m L. × 1.2 mm I.D. 2 μm film thickness
Flow rate: He 20 mL/min
C.Temperature: 60°C
Detection: FID
Injection volume: 1 μL
System: -