

## 水中の低級脂肪酸の分析

## Analysis of Short chain fatty acids in water

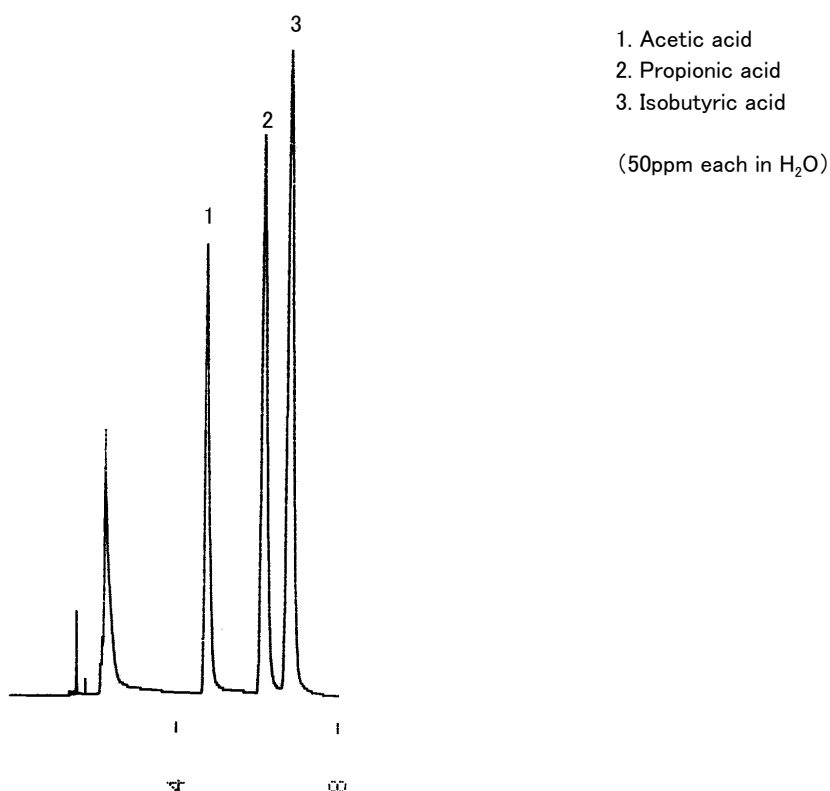


Fig. Chromatogram of Short chain fatty acids in water.

## 【Analytical conditions】

Column: **G-column G-300** 40 m L. × 1.2 mm I.D. 1 μm film thickness  
Flow rate: He 20 mL/min  
C.Temperature: 130°C  
Detection: FID  
Injection volume: 1 μL  
System: