

有機ハロゲン化合物の分析

Analysis of Organic halides

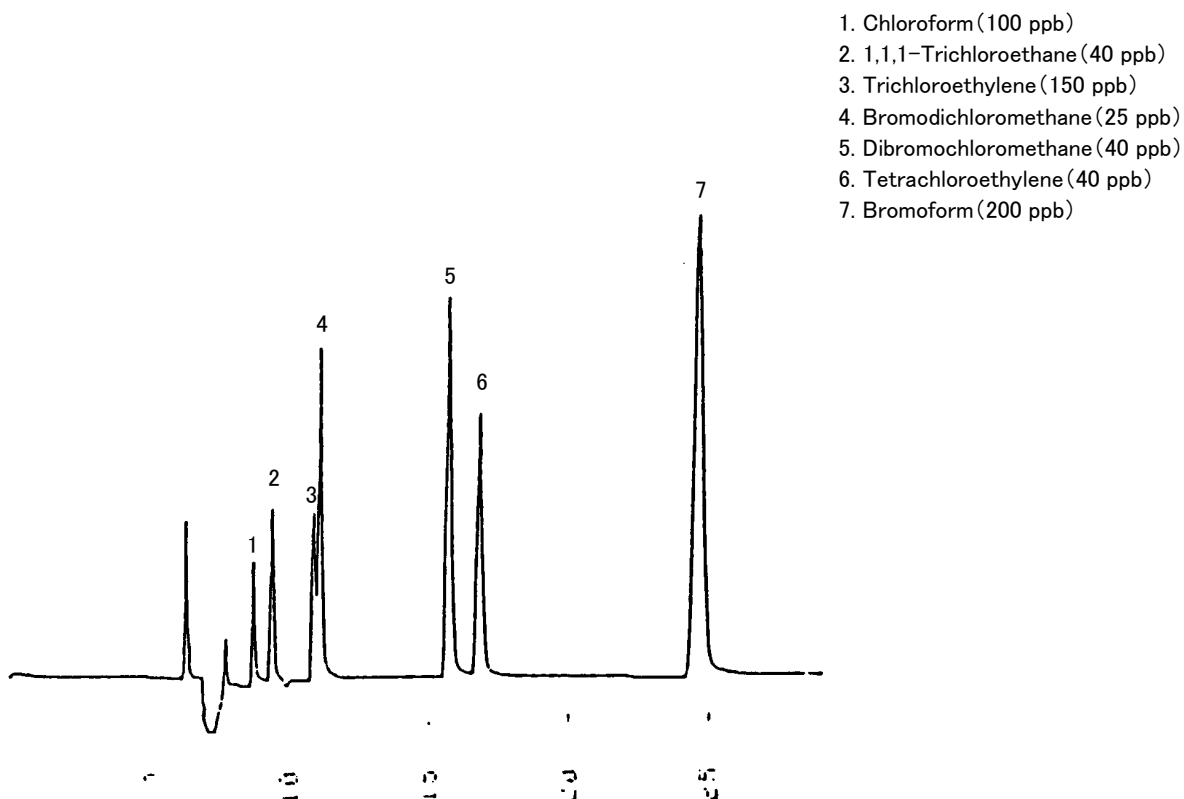


Fig. Chromatogram of Organic halides.

【Analytical conditions】

Column: **G-column G-205** 40 m L. × 1.2 mm I.D. 2 μ m film thickness
Flow rate: He 30 mL/min, Make-up gas N₂ 25 mL/min
C.Temperature: 80°C
Detection: ECD
Injection volume: 1 μ L
System: -