

脂肪酸の分析

Analysis of Fatty acids

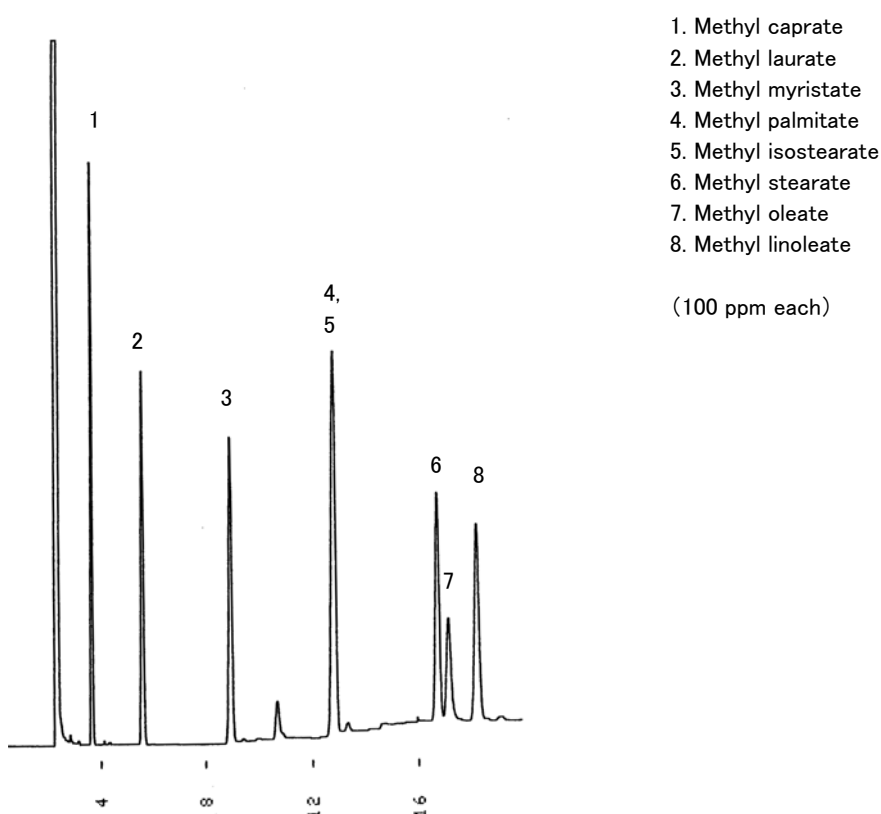


Fig. Chromatogram of Fatty acids.

【Analytical conditions】

Column: **G-column G-300** 40 m L. × 1.2 mm I.D. 0.5 μ m film thickness
Flow rate: He 20 mL/min
C.Temperature: 150°C (5 min hold) → 5°C/min → 200°C
Detection: FID
Injection volume: 1 μ L
System: -