

作業環境中の有機溶剤の分析

Analysis of Organic solvents in working environment assessment

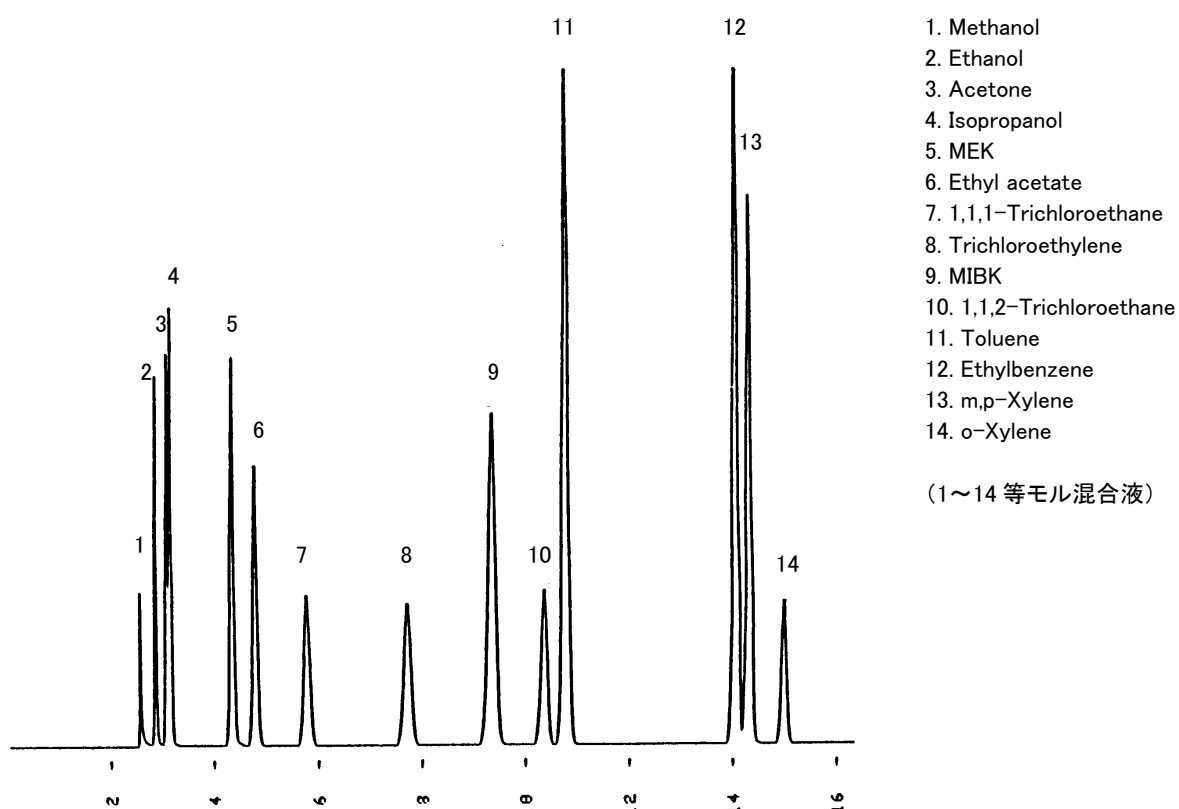


Fig. Chromatogram of Organic solvents in working environment assessment.

【Analytical conditions】

Column: **G-column G-100** 40 m L. × 1.2 mm I.D. 3 μm film thickness
Flow rate: He 19.5 mL/min
C.Temperature: 50°C (8 min hold) → 10°C/min → 110°C
Detection: FID
Injection volume: 0.2 μL
System: GC-9A (Shimadzu Co.)