

有機溶剤中の微量成分(メタノール中のアセトン)の分析

Analysis of Trace constitutes in organic solvent

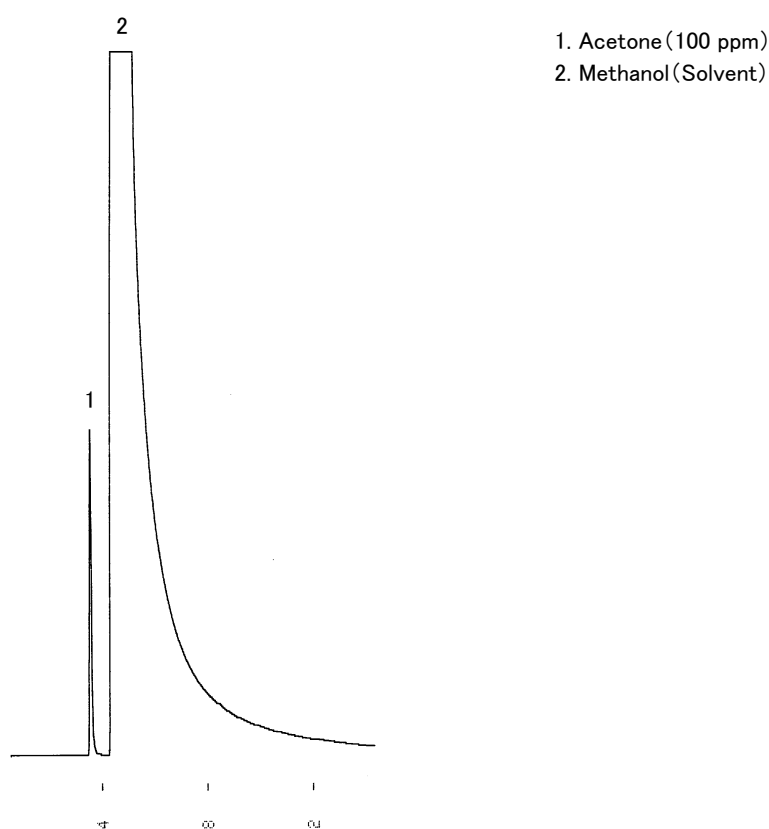


Fig. Chromatogram of Trace constitutes in organic solvent.

【Analytical conditions】

Column: **G-column G-300** 40 m L. × 1.2 mm I.D. 2 μm film thickness
Flow rate:
C.Temperature: 60°C
Detection: FID
Injection volume: 2 μL
System: GC-9A (Shimadzu Co.)