

水中の低級アルコールの分析

Analysis of Lower alcohols in water

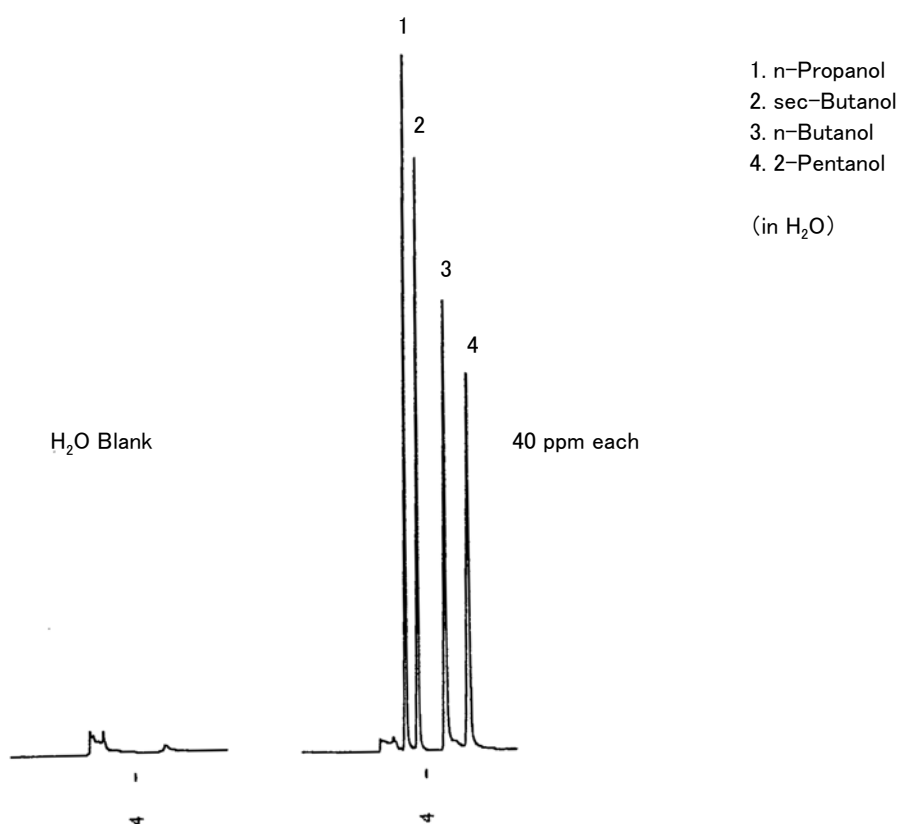


Fig. Chromatogram of lower alcohols in water.

【Analytical conditions】

Column:	G-column G-205 40 m L. × 1.2 mm I.D. 2 μm film thickness
Flow rate:	He 20 mL/min
C.Temperature:	60°C
Detection:	FID
Injection volume:	1 μL
System:	-