

水中の低級脂肪酸の分析

Analysis of Short chain fatty acids in water

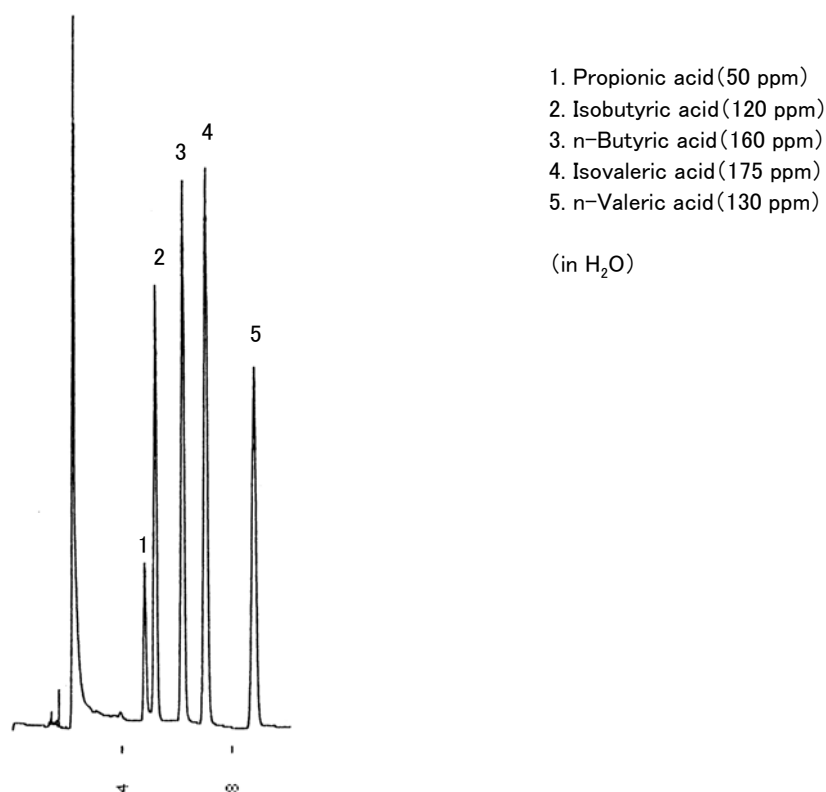


Fig. Chromatogram of short chain fatty acids in water.

【Analytical conditions】

Column: **G-column G-300** 40 m L. × 1.2 mm I.D. 1 μm film thickness
Flow rate: He 20 mL/min
C.Temperature: 140°C
Detection: FID
Injection volume: 1 μL
System: GC-9A (Shimadzu Co.)