

## 水中の低級脂肪酸の分析

## Analysis of Short chain fatty acids in water

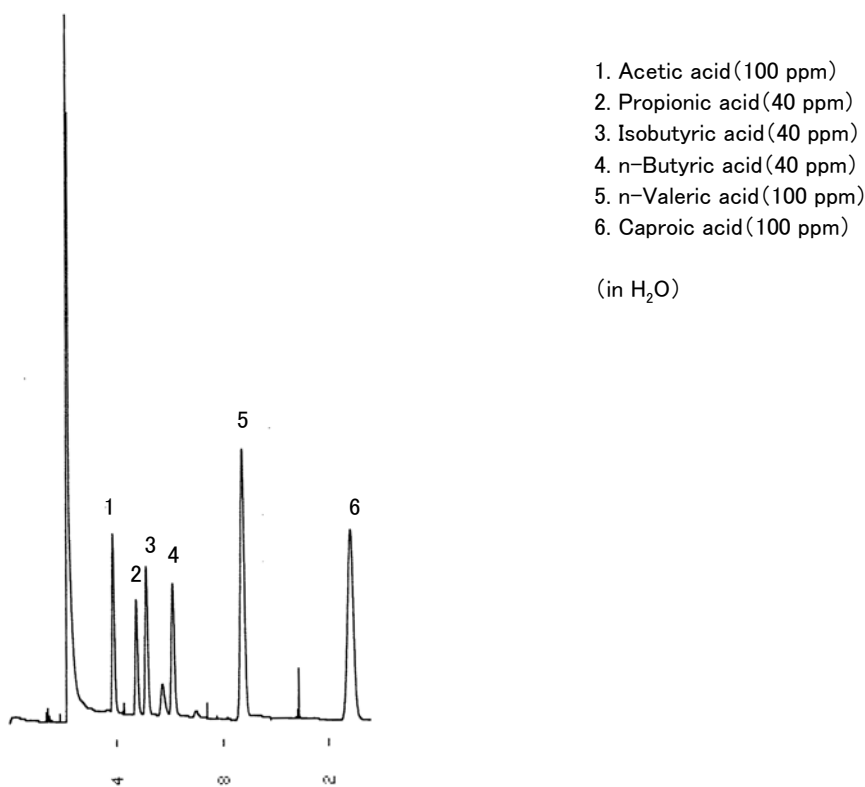


Fig. Chromatogram of short chain fatty acids in water.

## 【Analytical conditions】

Column:	<b>G-column G-300</b> 40 m L. × 1.2 mm I.D. 1 μm film thickness
Flow rate:	He 20 mL/min
C.Temperature:	140°C
Detection:	FID
Injection volume:	1 μL
System:	GC-9A (Shimadzu Co.)