

市販軟膏の分析

Analysis of Ointment

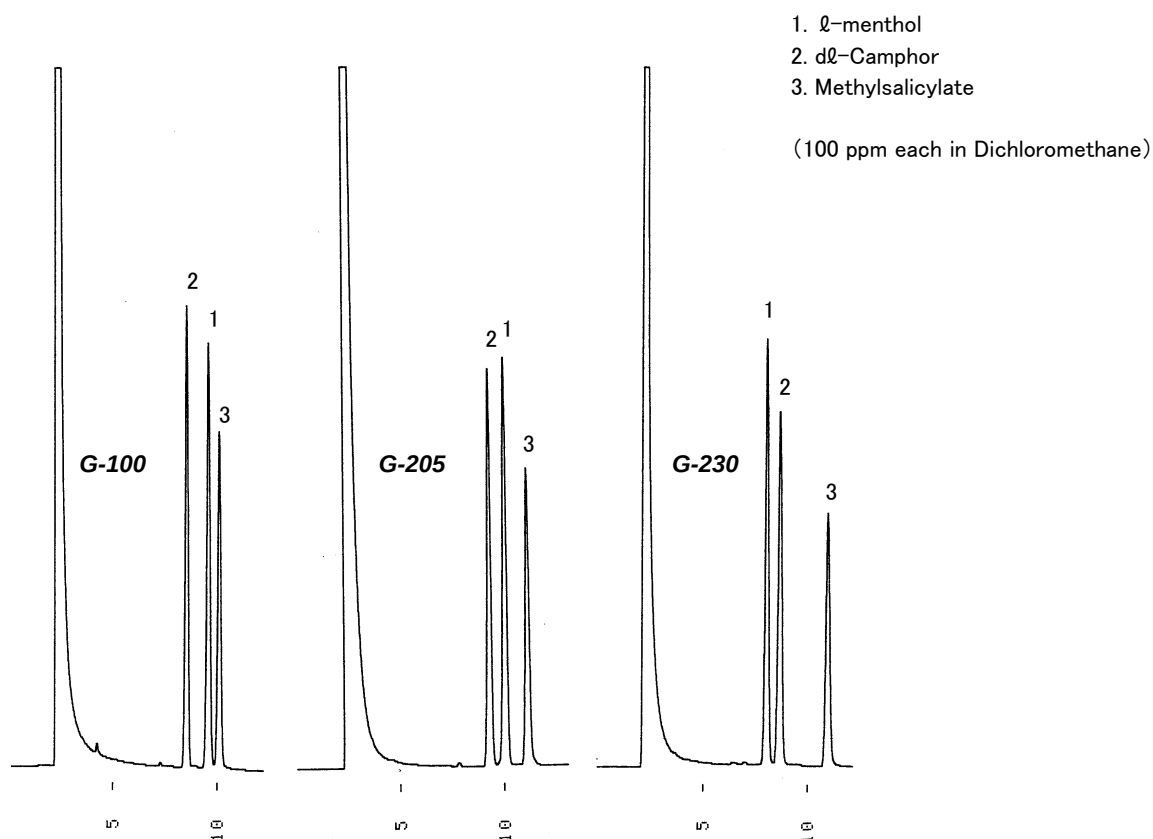


Fig. Chromatogram of Ointment.

【Analytical conditions】

Column: **G-column G-100,G-205,G-230** 40 m L. × 1.2 mm I.D. 2 μm film thickness
Flow rate: He 20 mL/min
C.Temperature: 130°C
Detection: FID
Injection volume: 1 μL
System: -